



Compression/ Distraction Device for Ankle Fix System, 0-15 mm 28.14.000

Cleaning Instructions

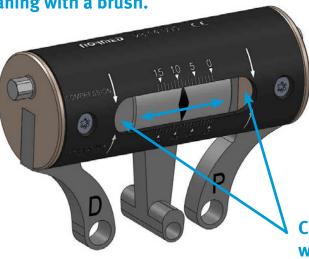

Clean parts marked with the arrows.

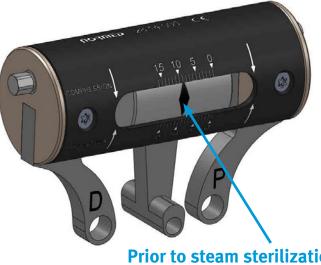

Prior to steam sterilization, set the cylinder in the central position.

97-8779-094-00 ©2015 Zimmer, Inc.



Set cylinder to both end positions while cleaning with a brush.